

**Straightness of Micro-hole**

Sample Lot; FBn1928K02D

Instrument ; Concentricity Measuring

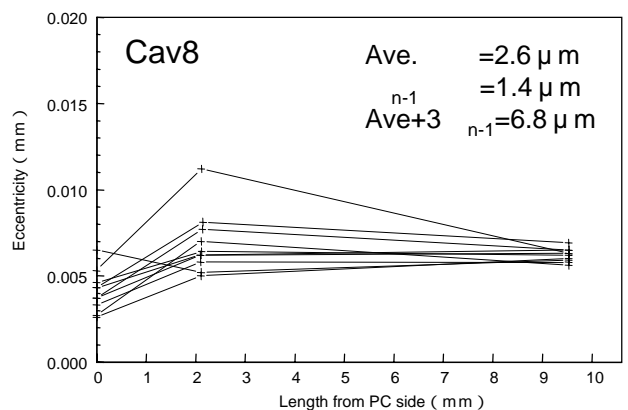
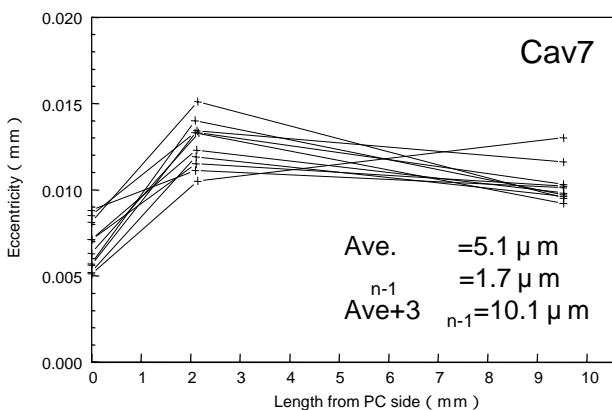
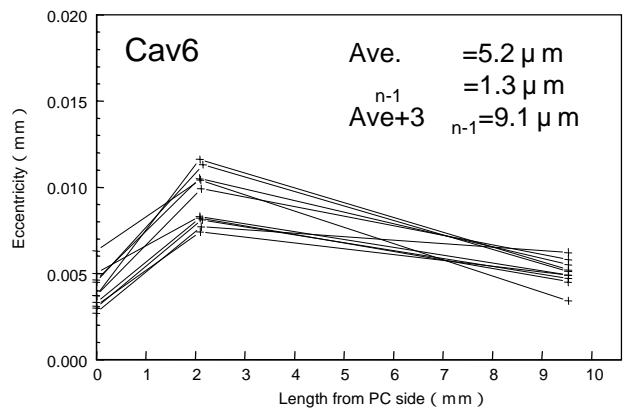
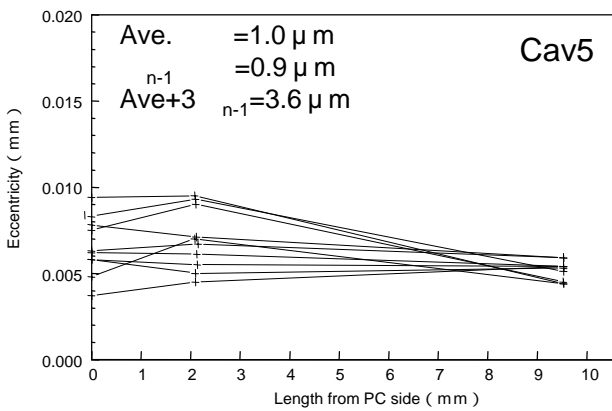
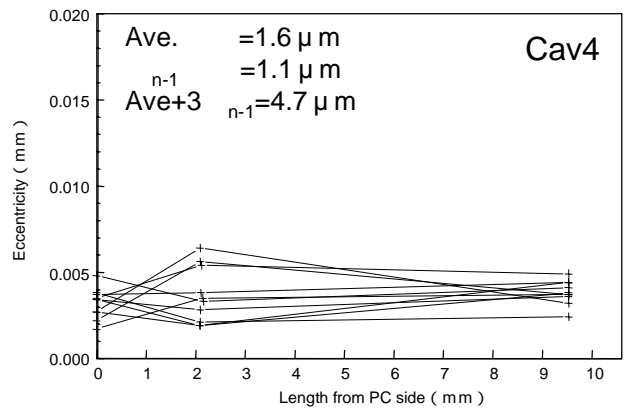
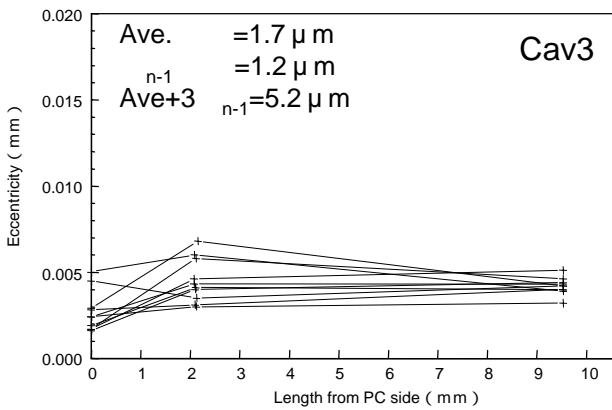
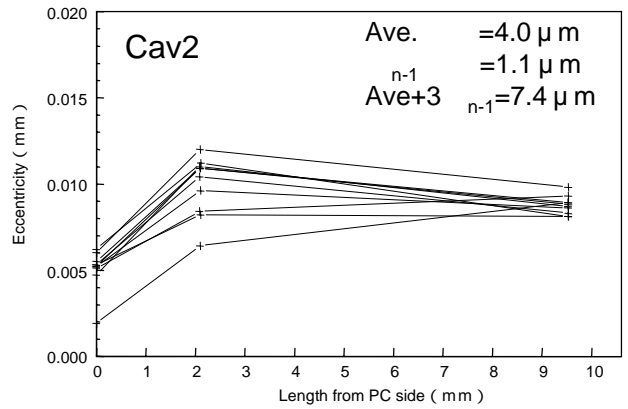
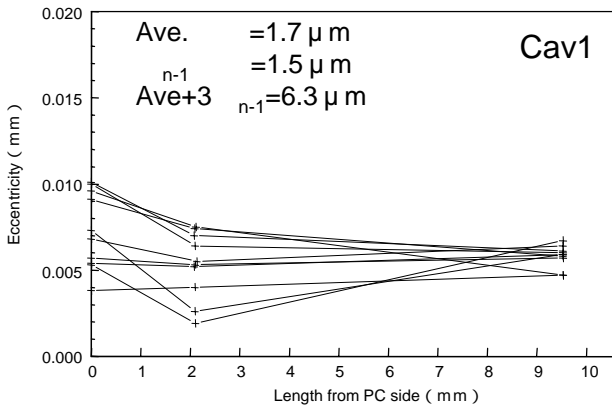


Fig.- Straightness of Micro-hole